

FIGURE 1

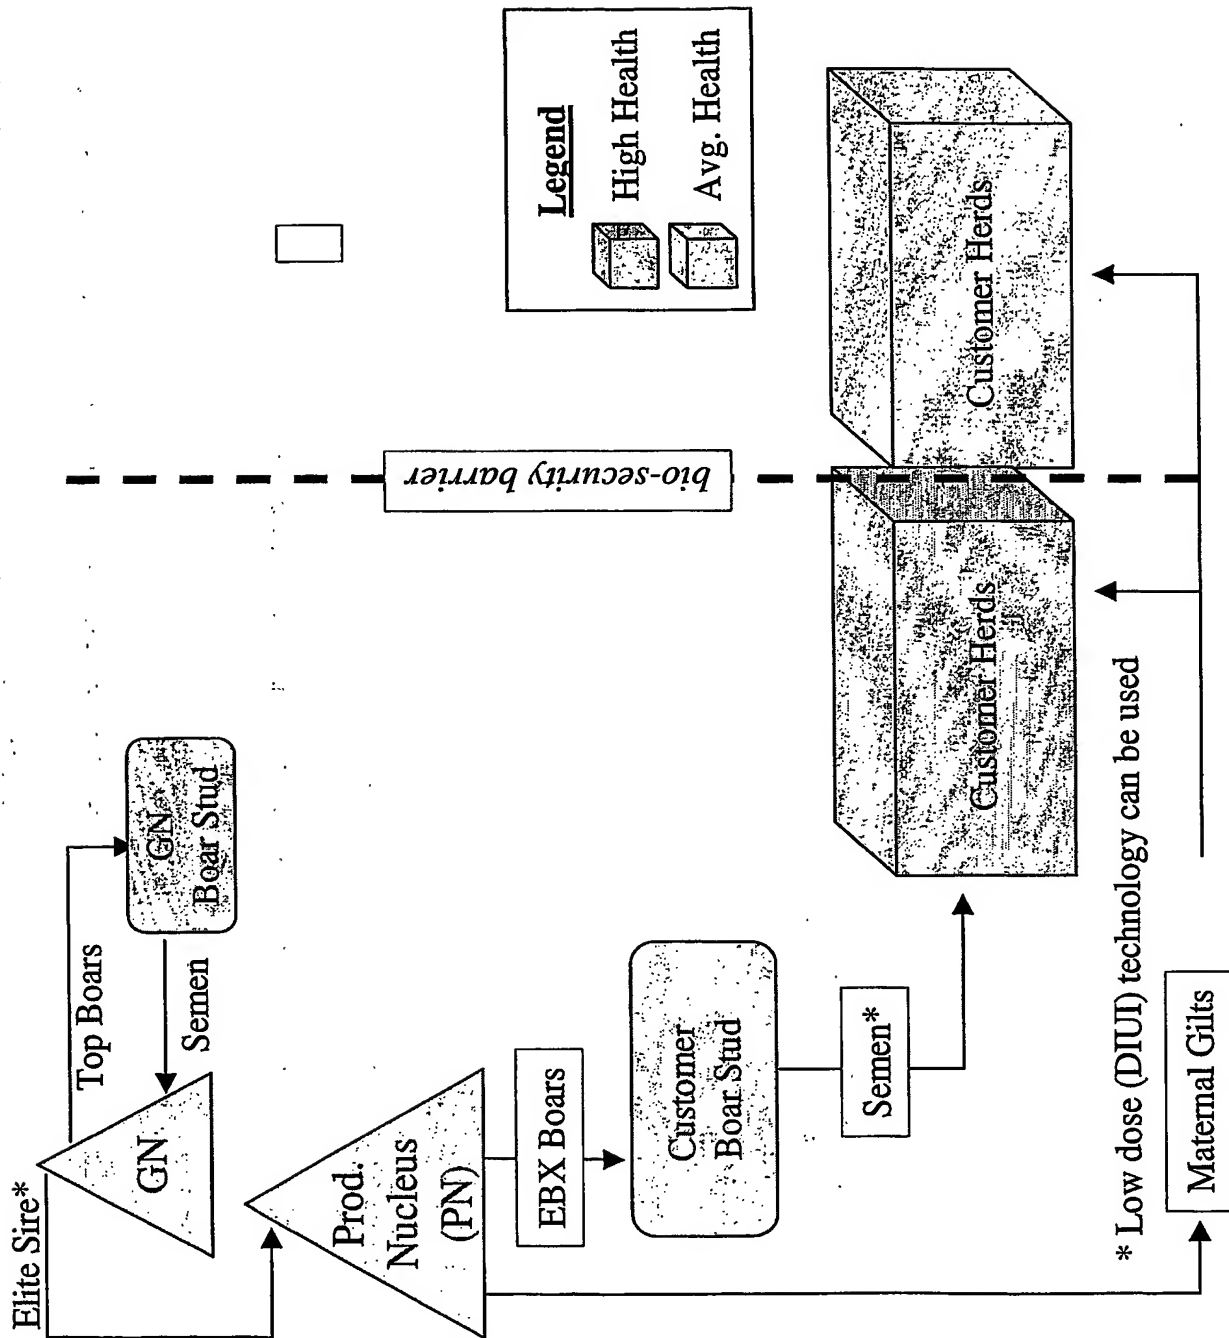
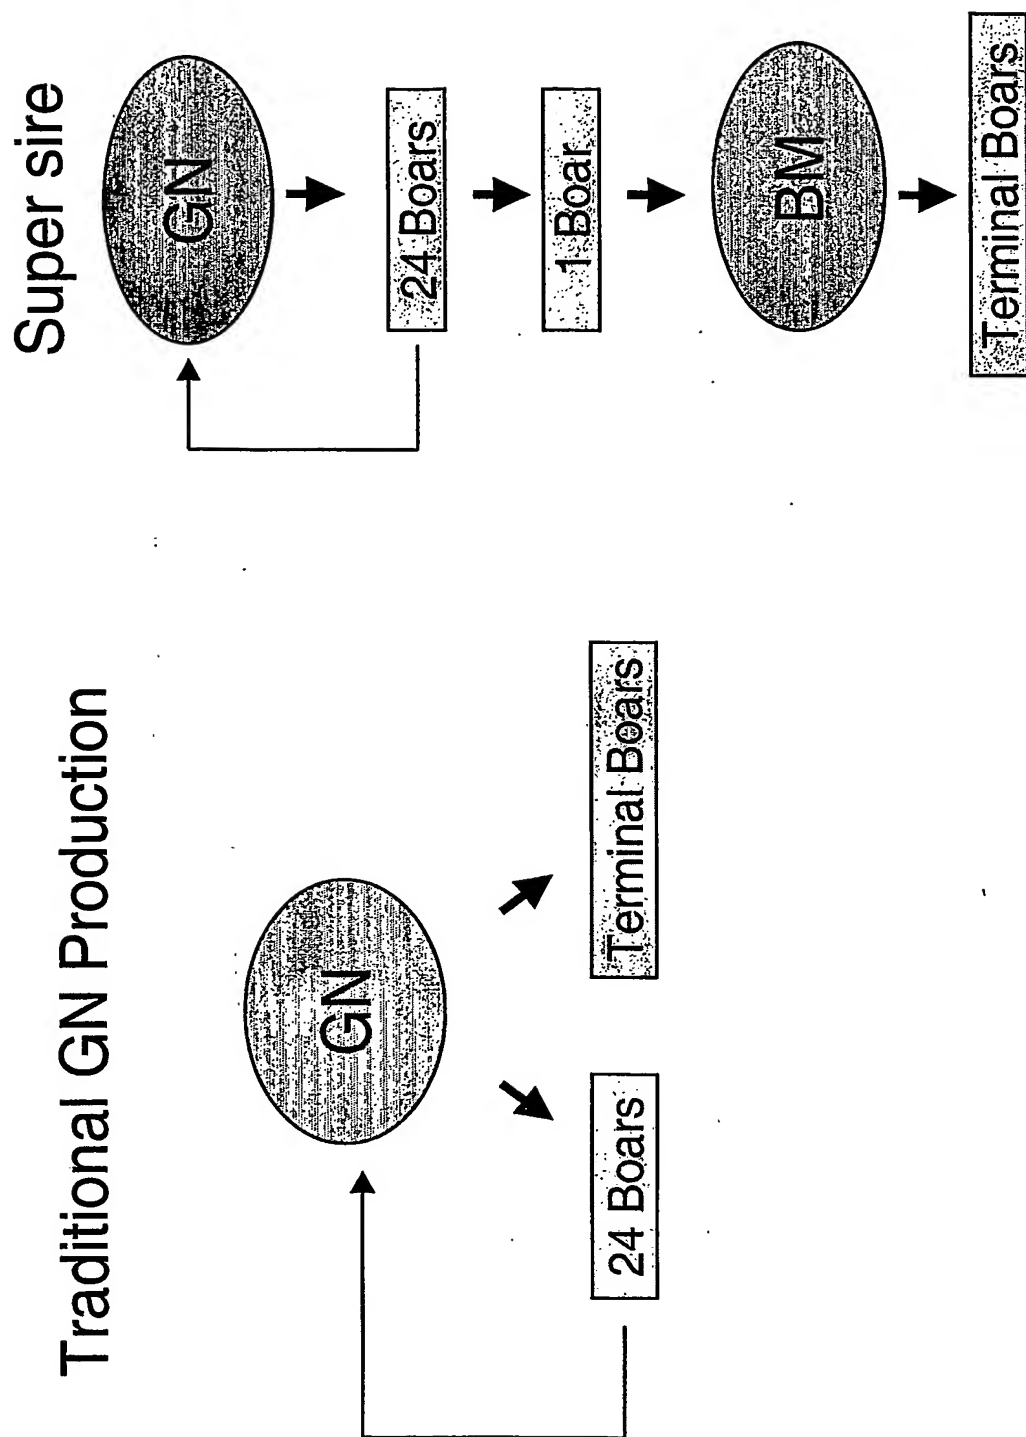
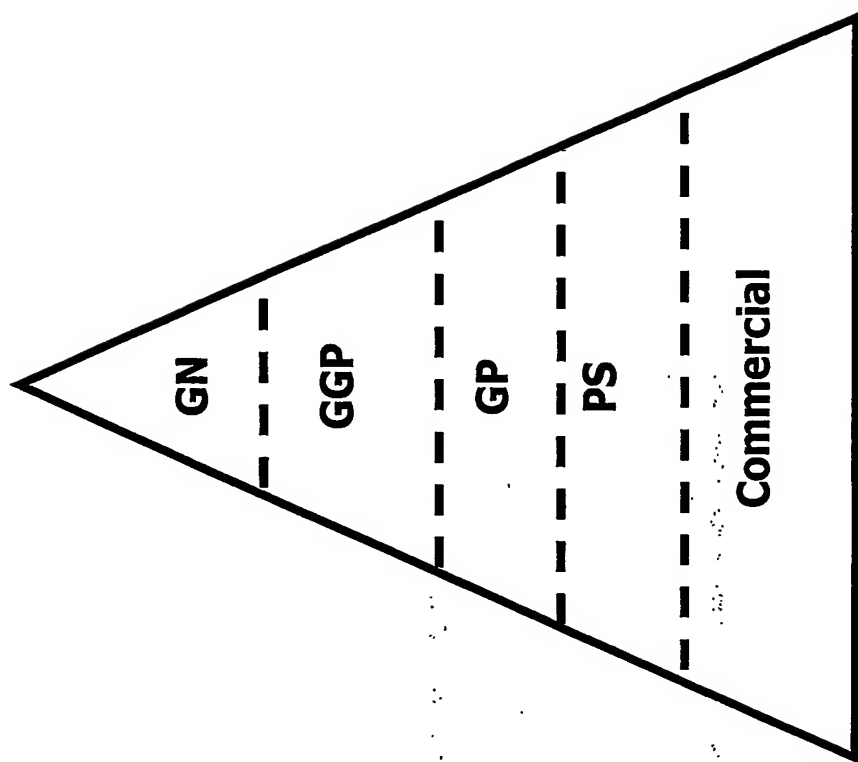


FIGURE 2

\* Low dose (DIUI) technology can be used



**FIGURE 3**



**FIGURE 4**

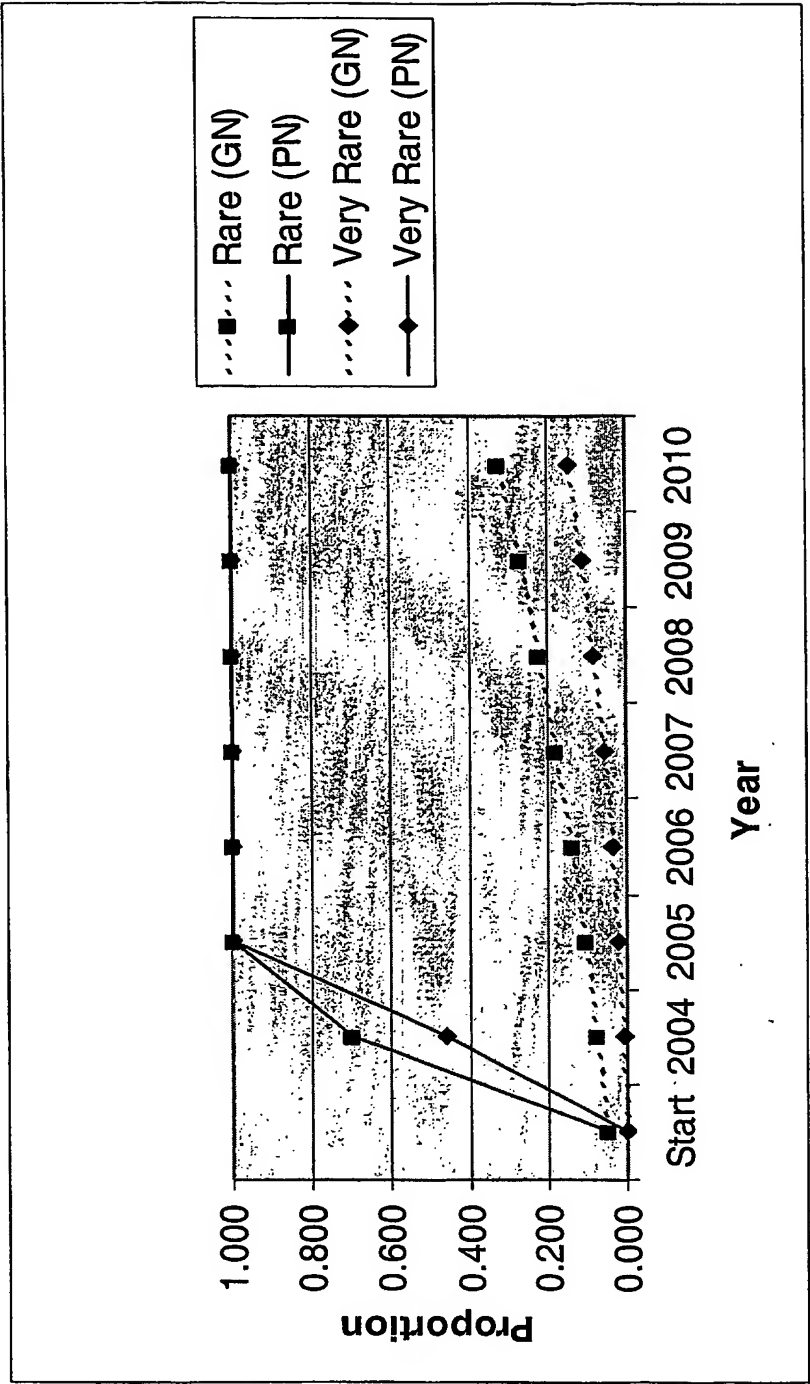


FIGURE 5

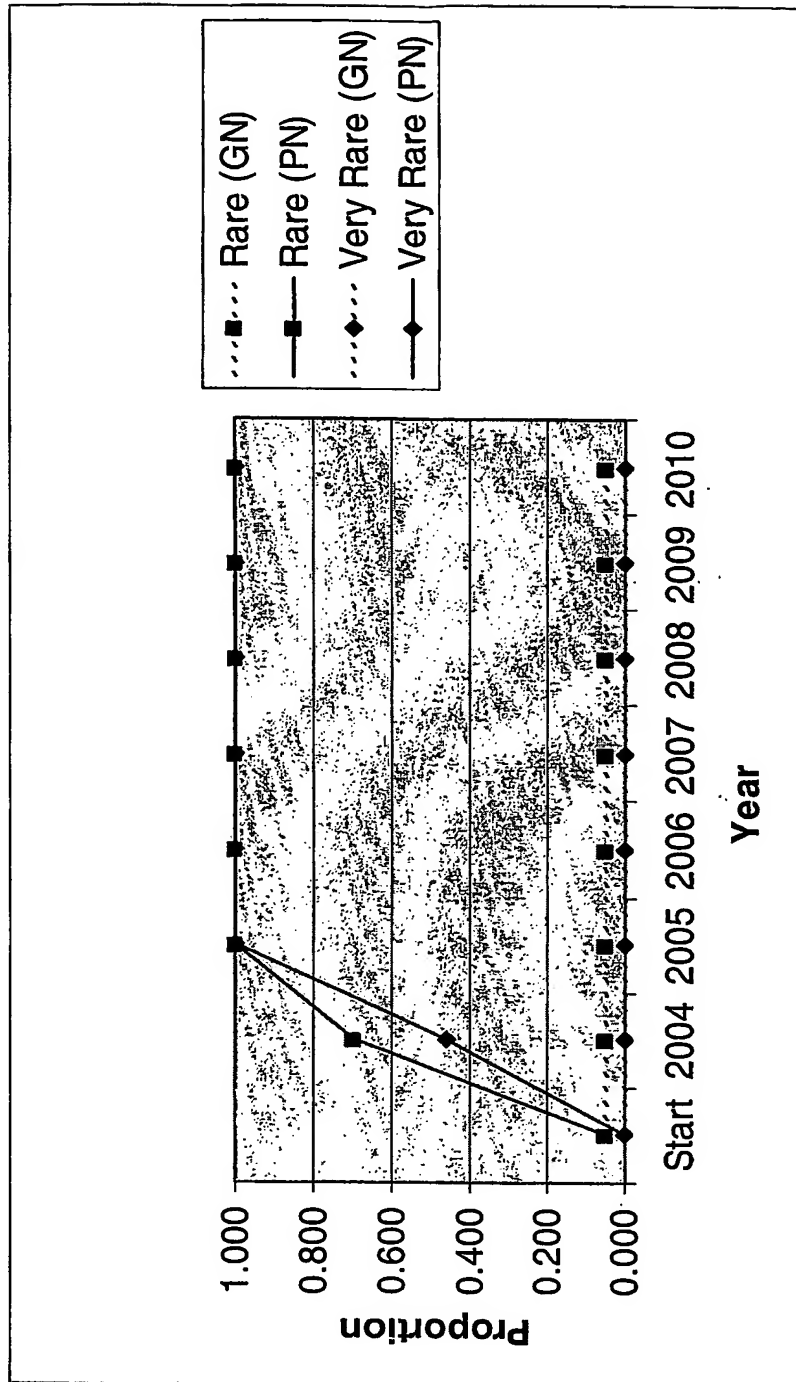


FIGURE 6


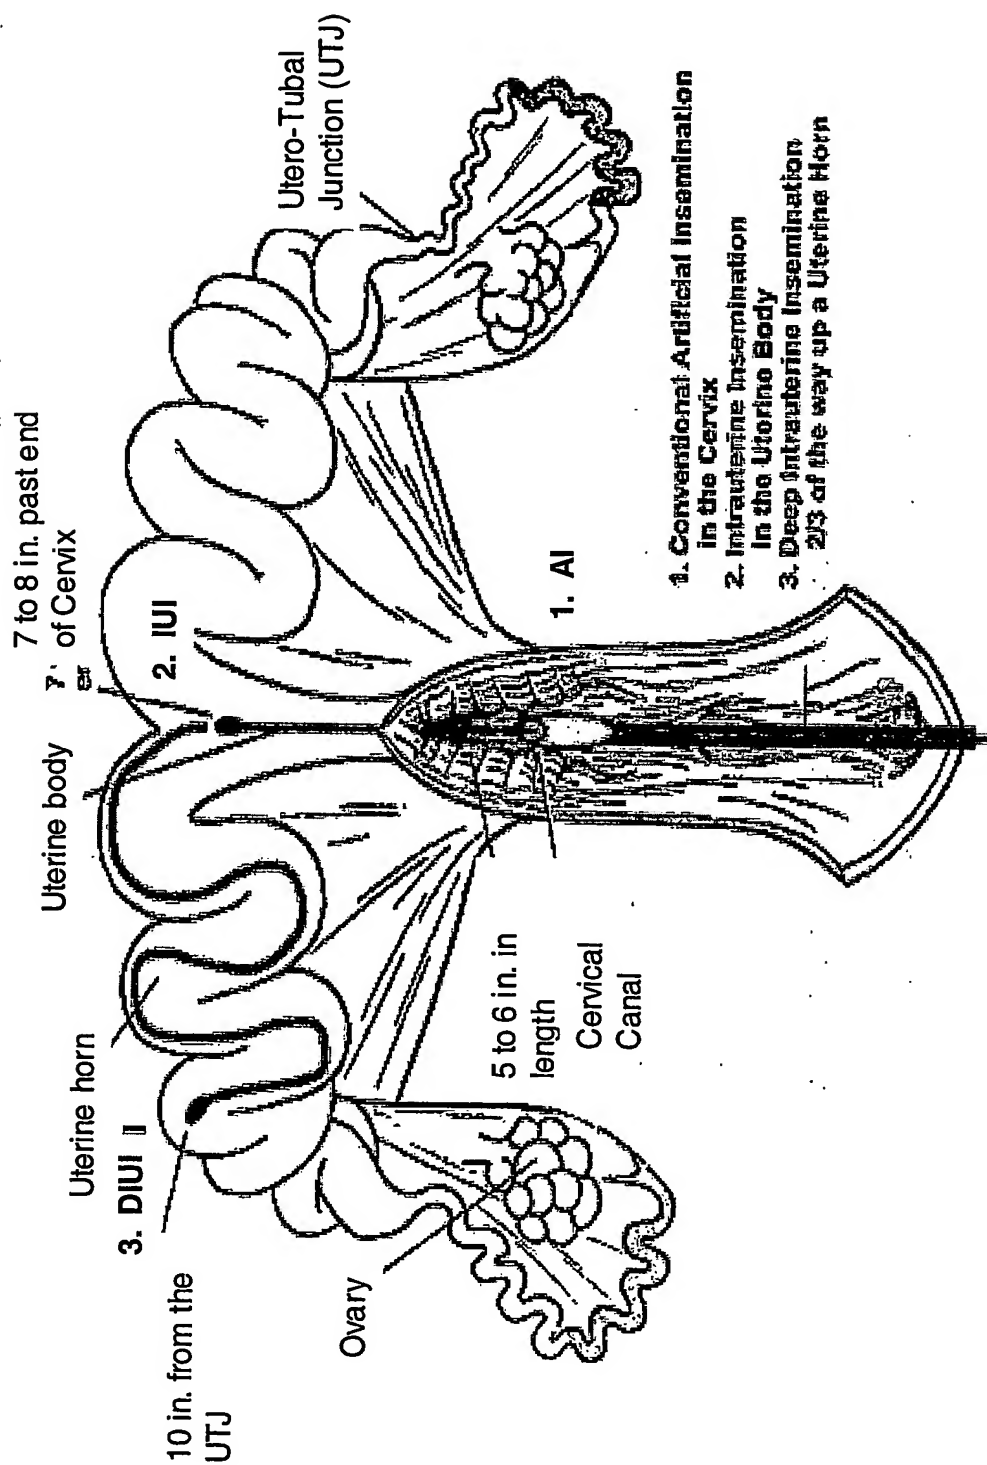


FIGURE 7

NOT AVAILABLE COPY


**FIGURE 8**




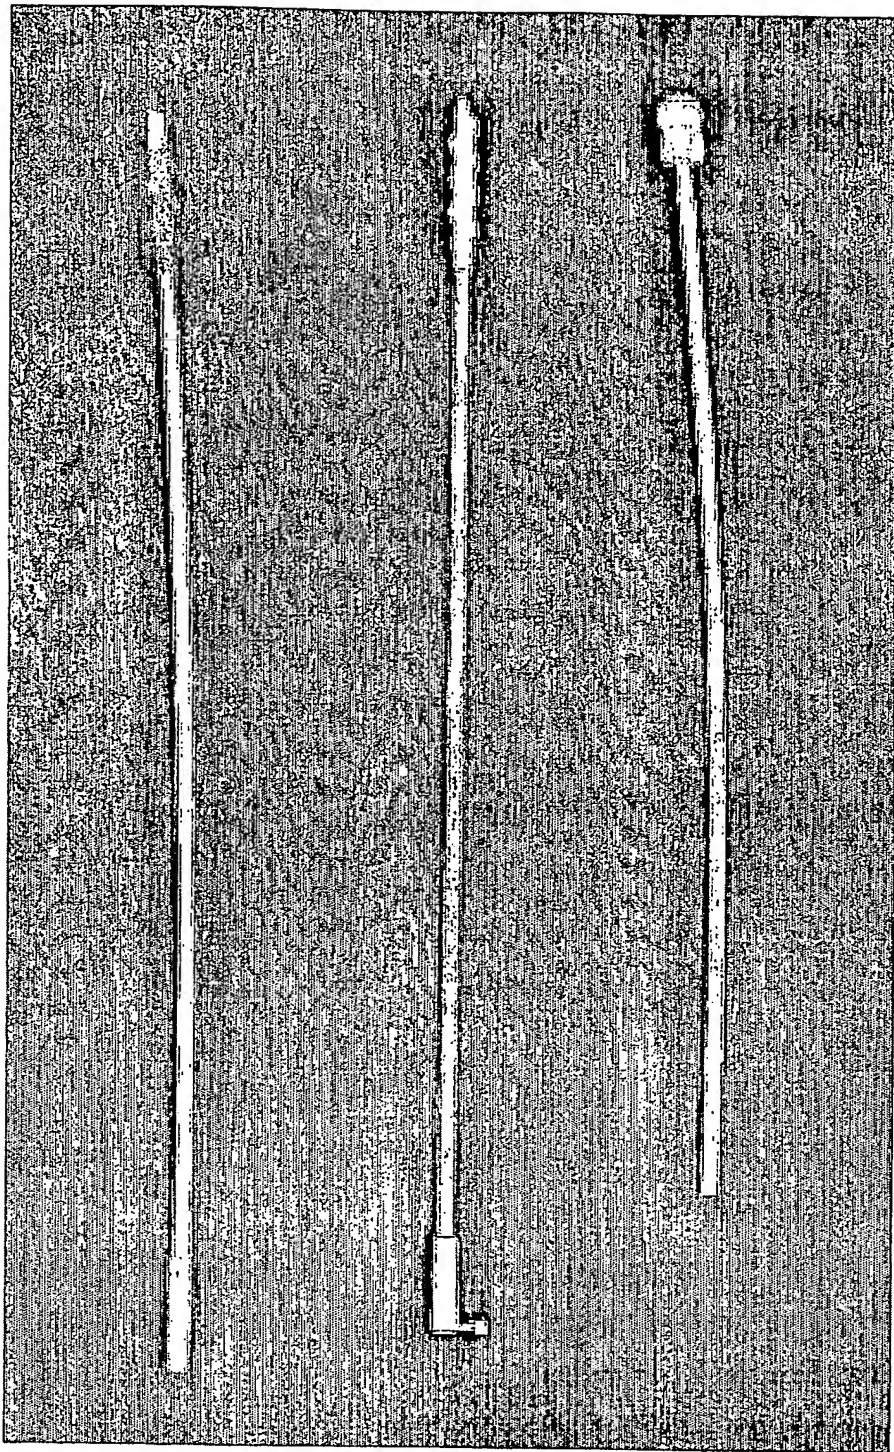

BEST AVAILABLE COPY

FIGURE 9

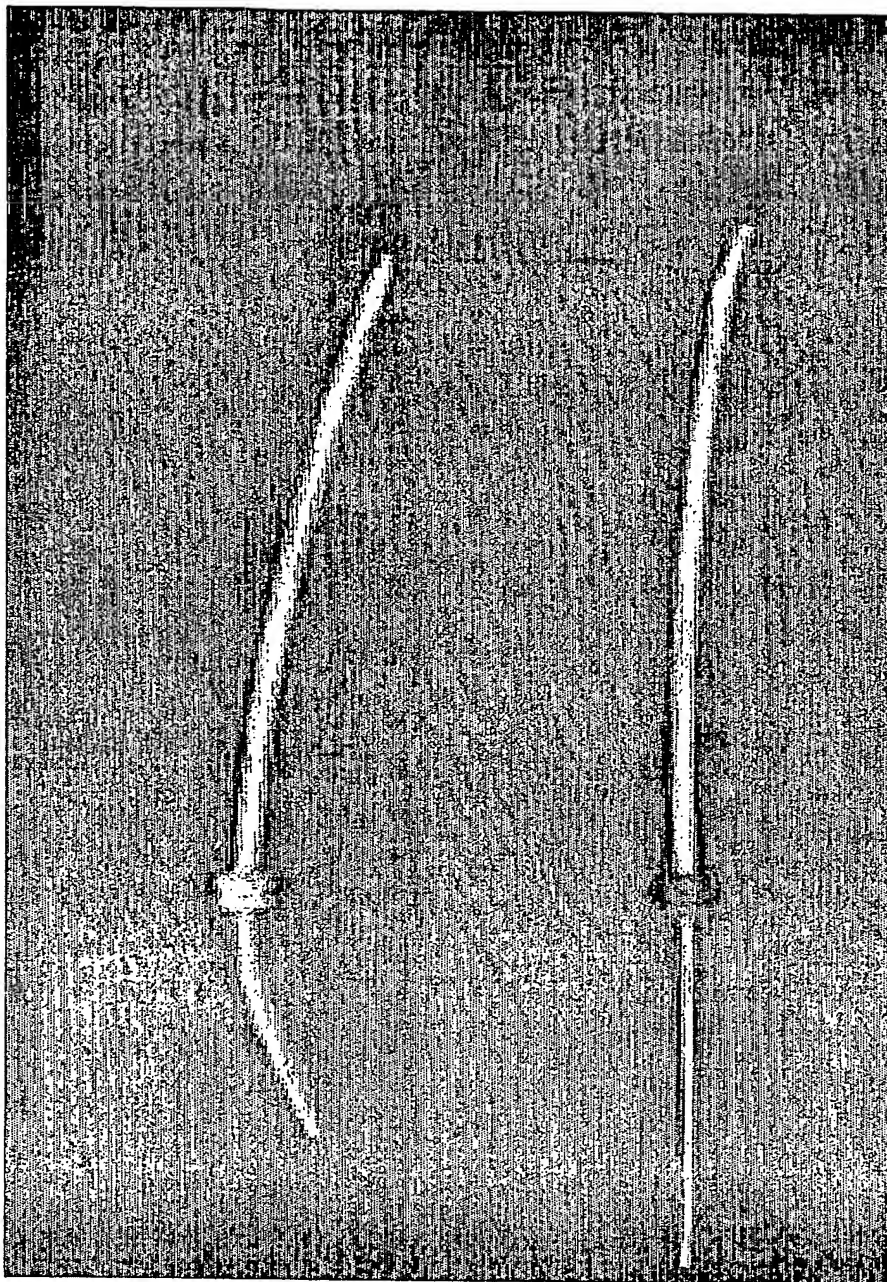

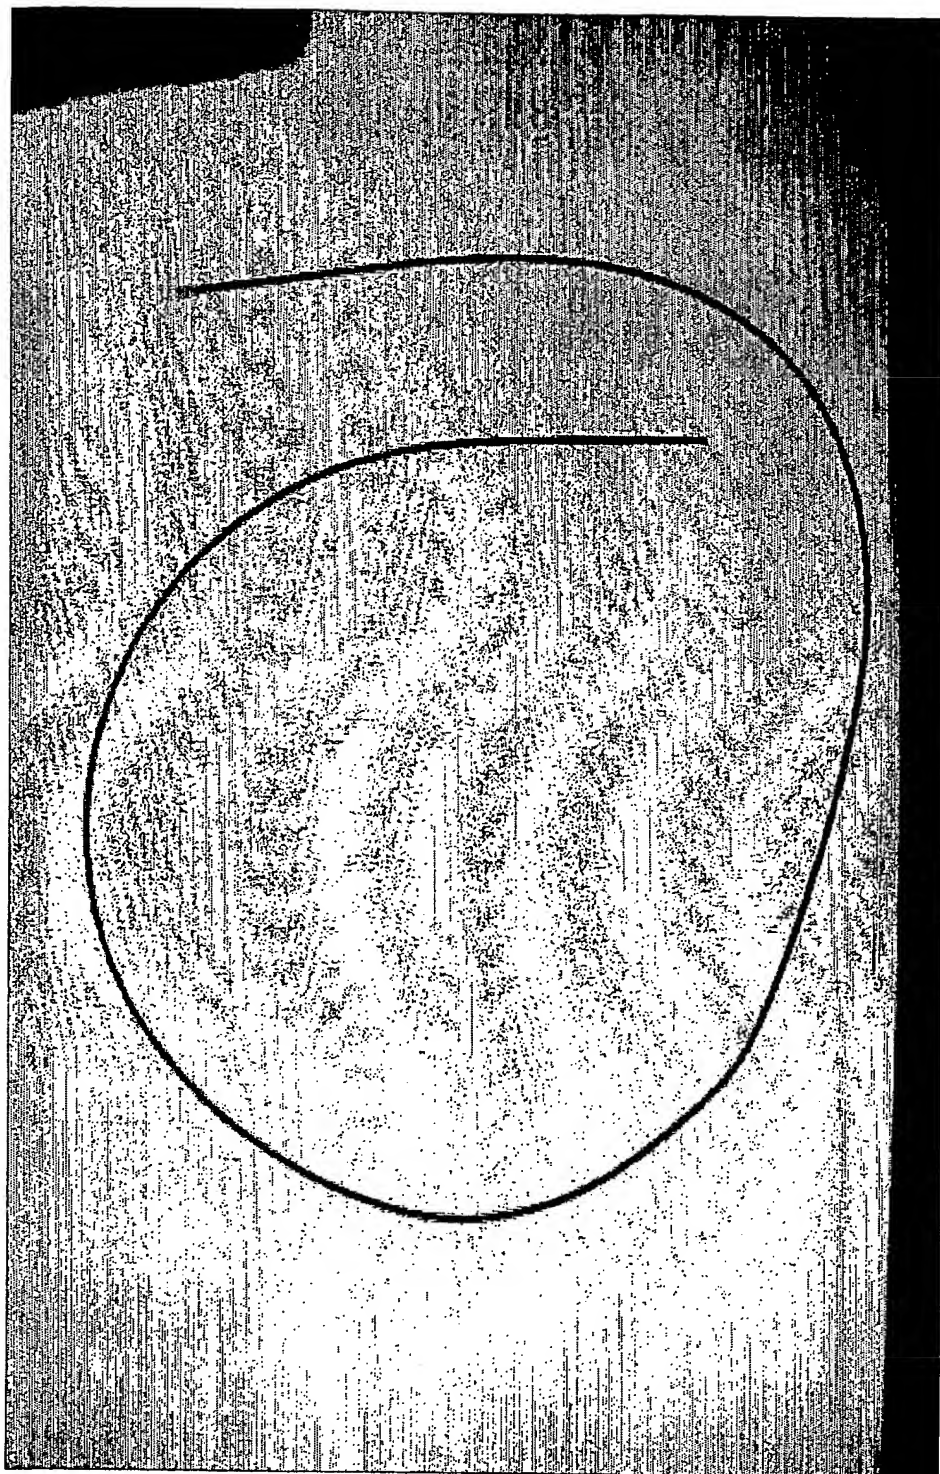

BEST AVAILABLE COPY  
FIGURE 10

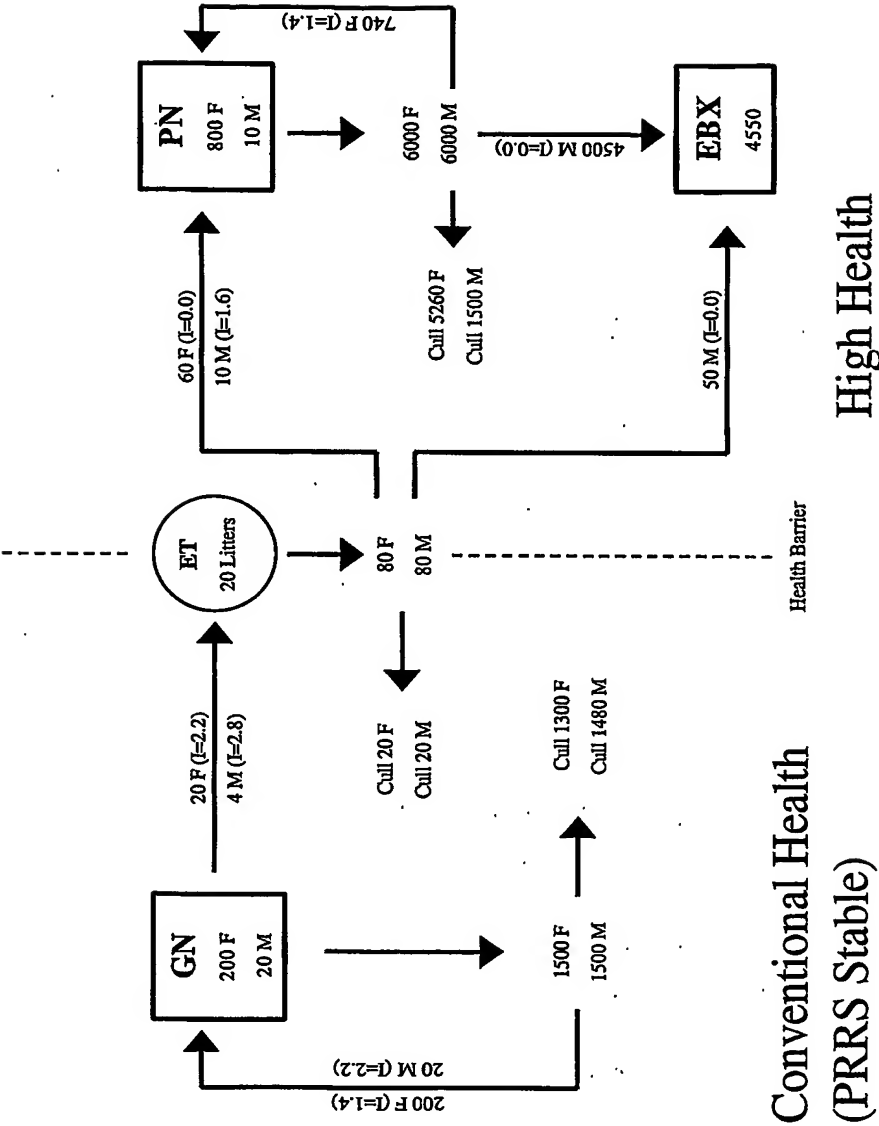


FIGURE 11

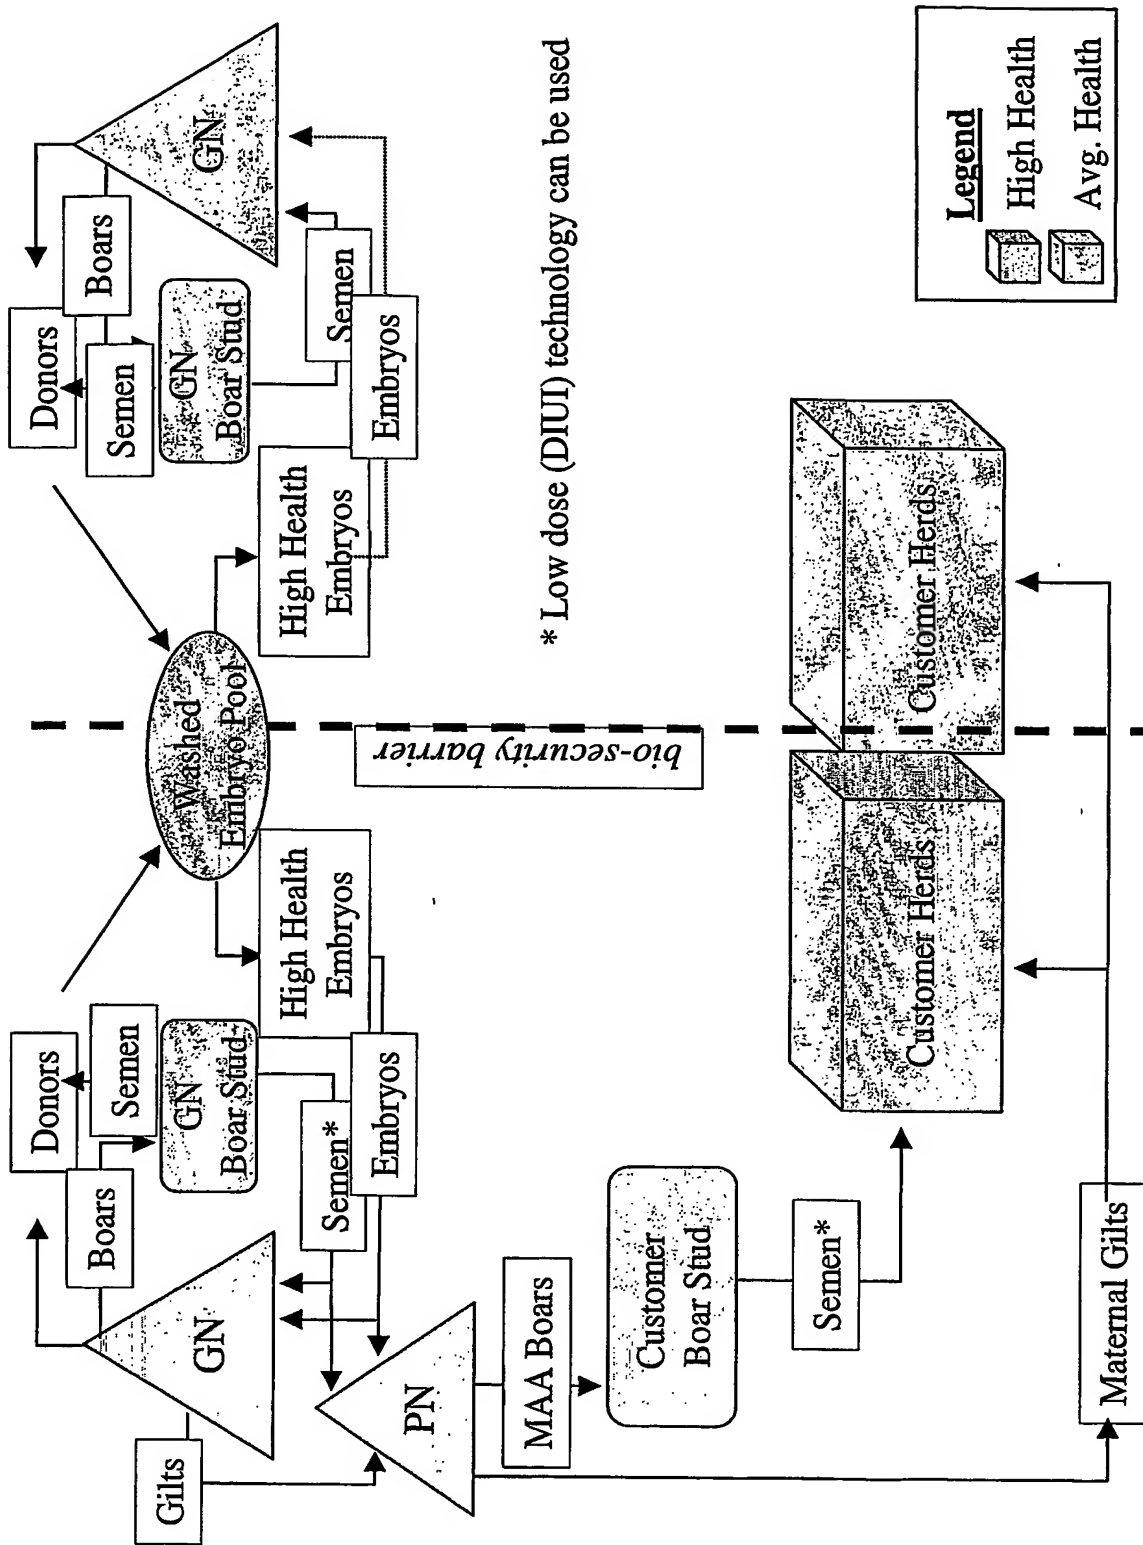


FIGURE 12


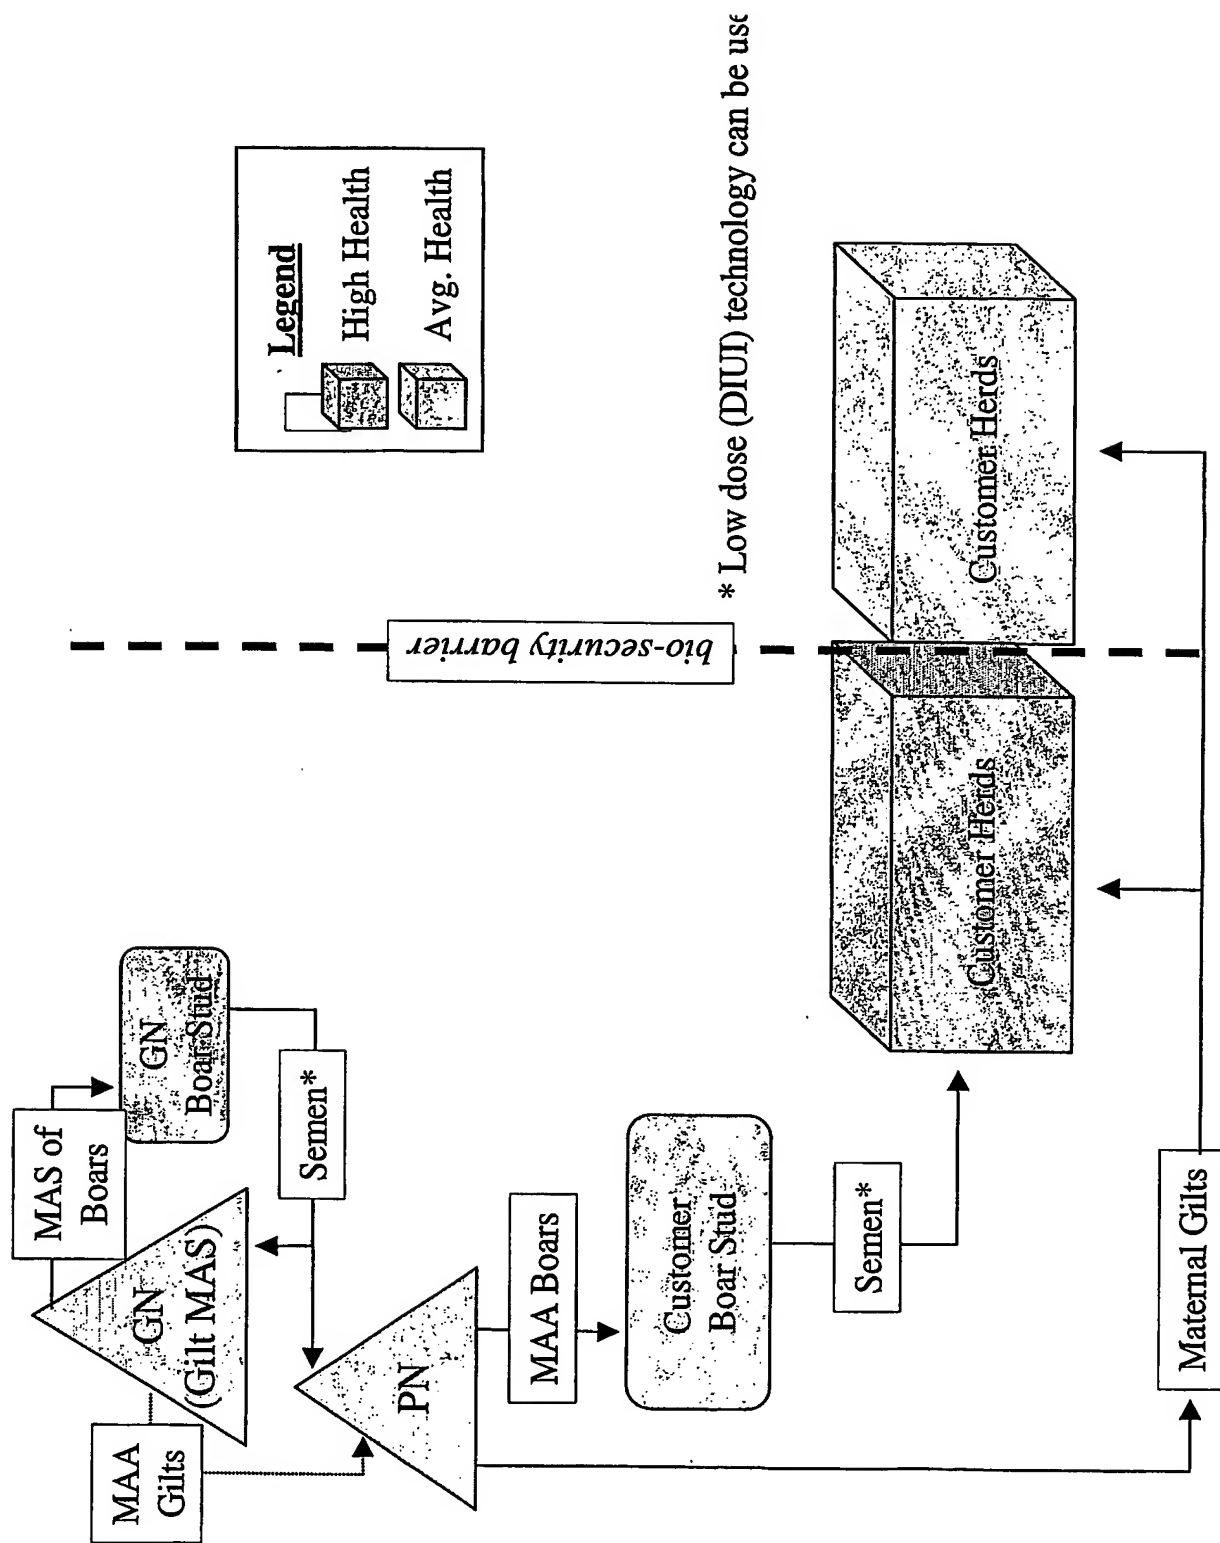


FIGURE 13

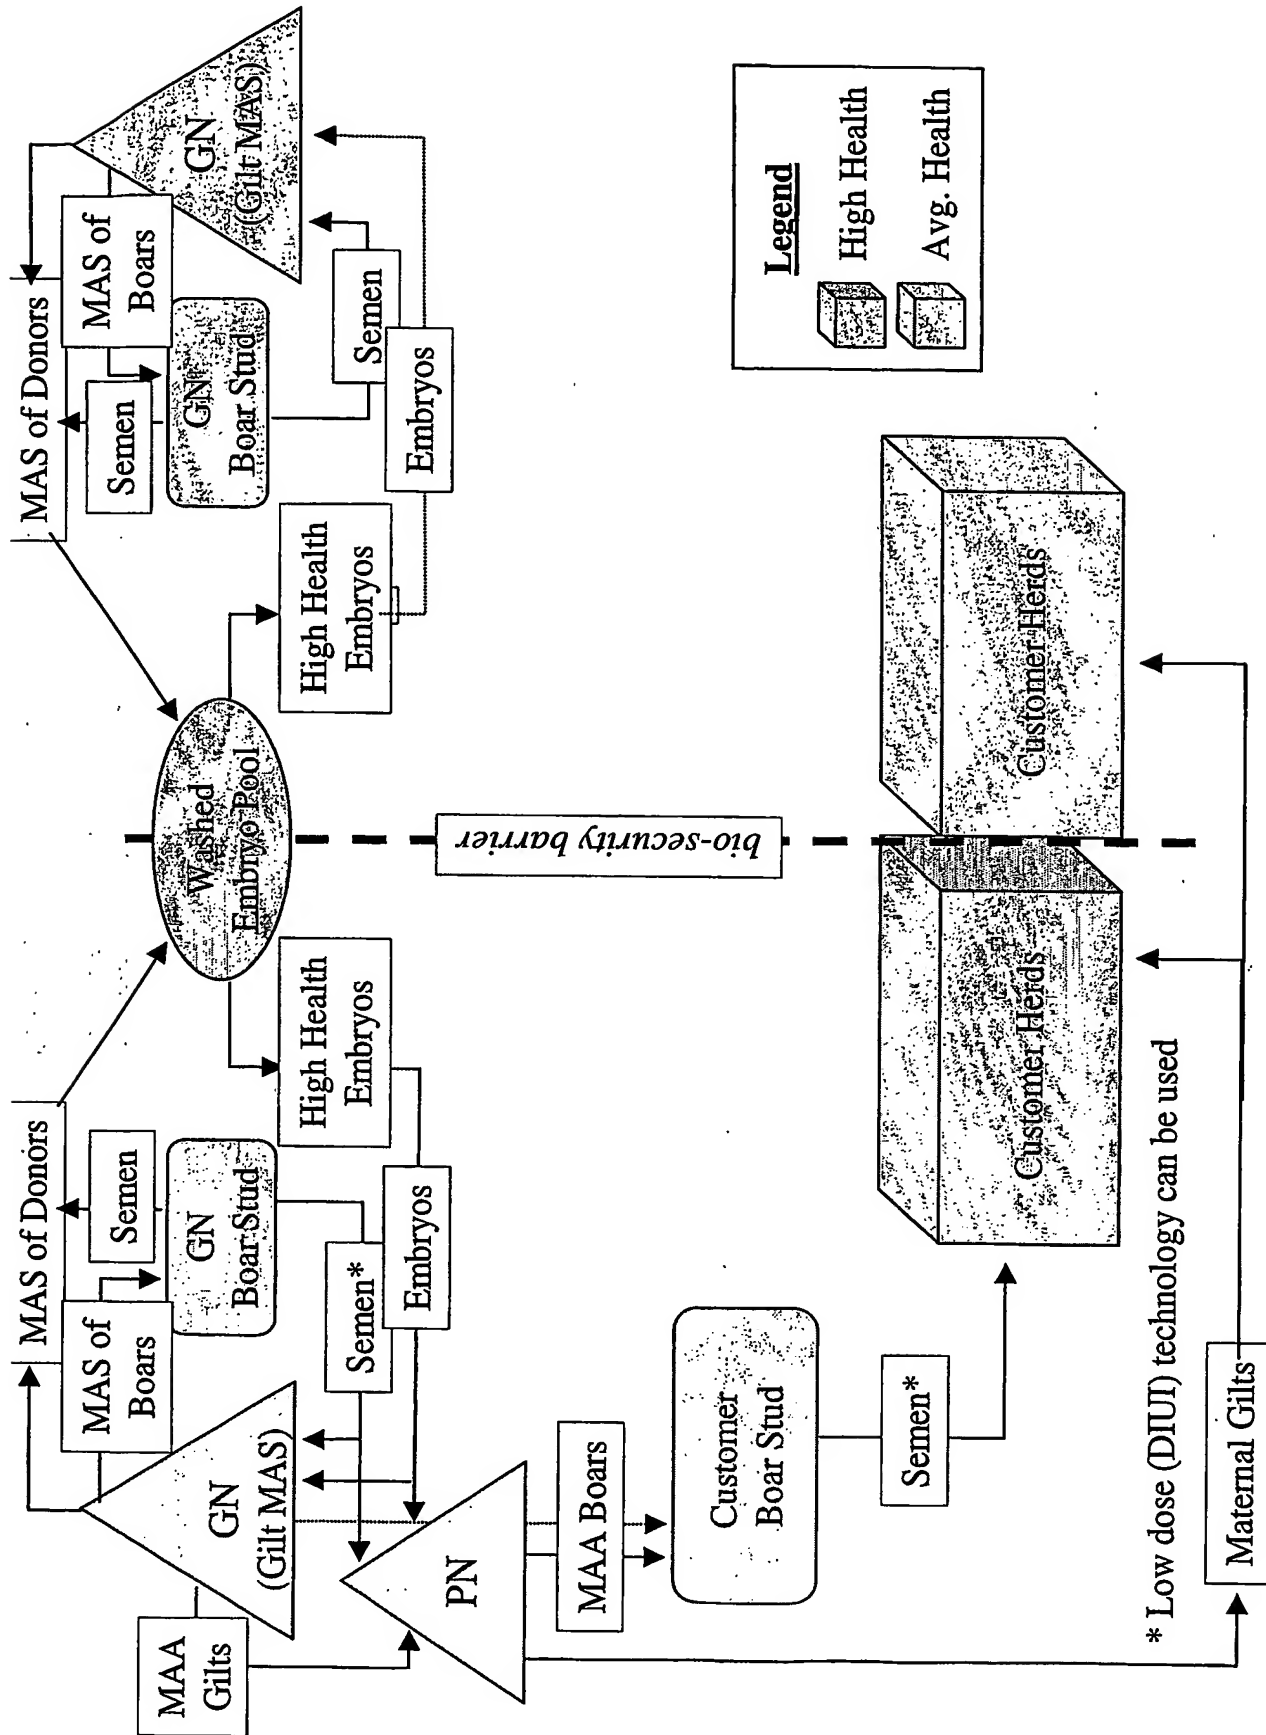

\* Low dose (DIUI) technology can be used

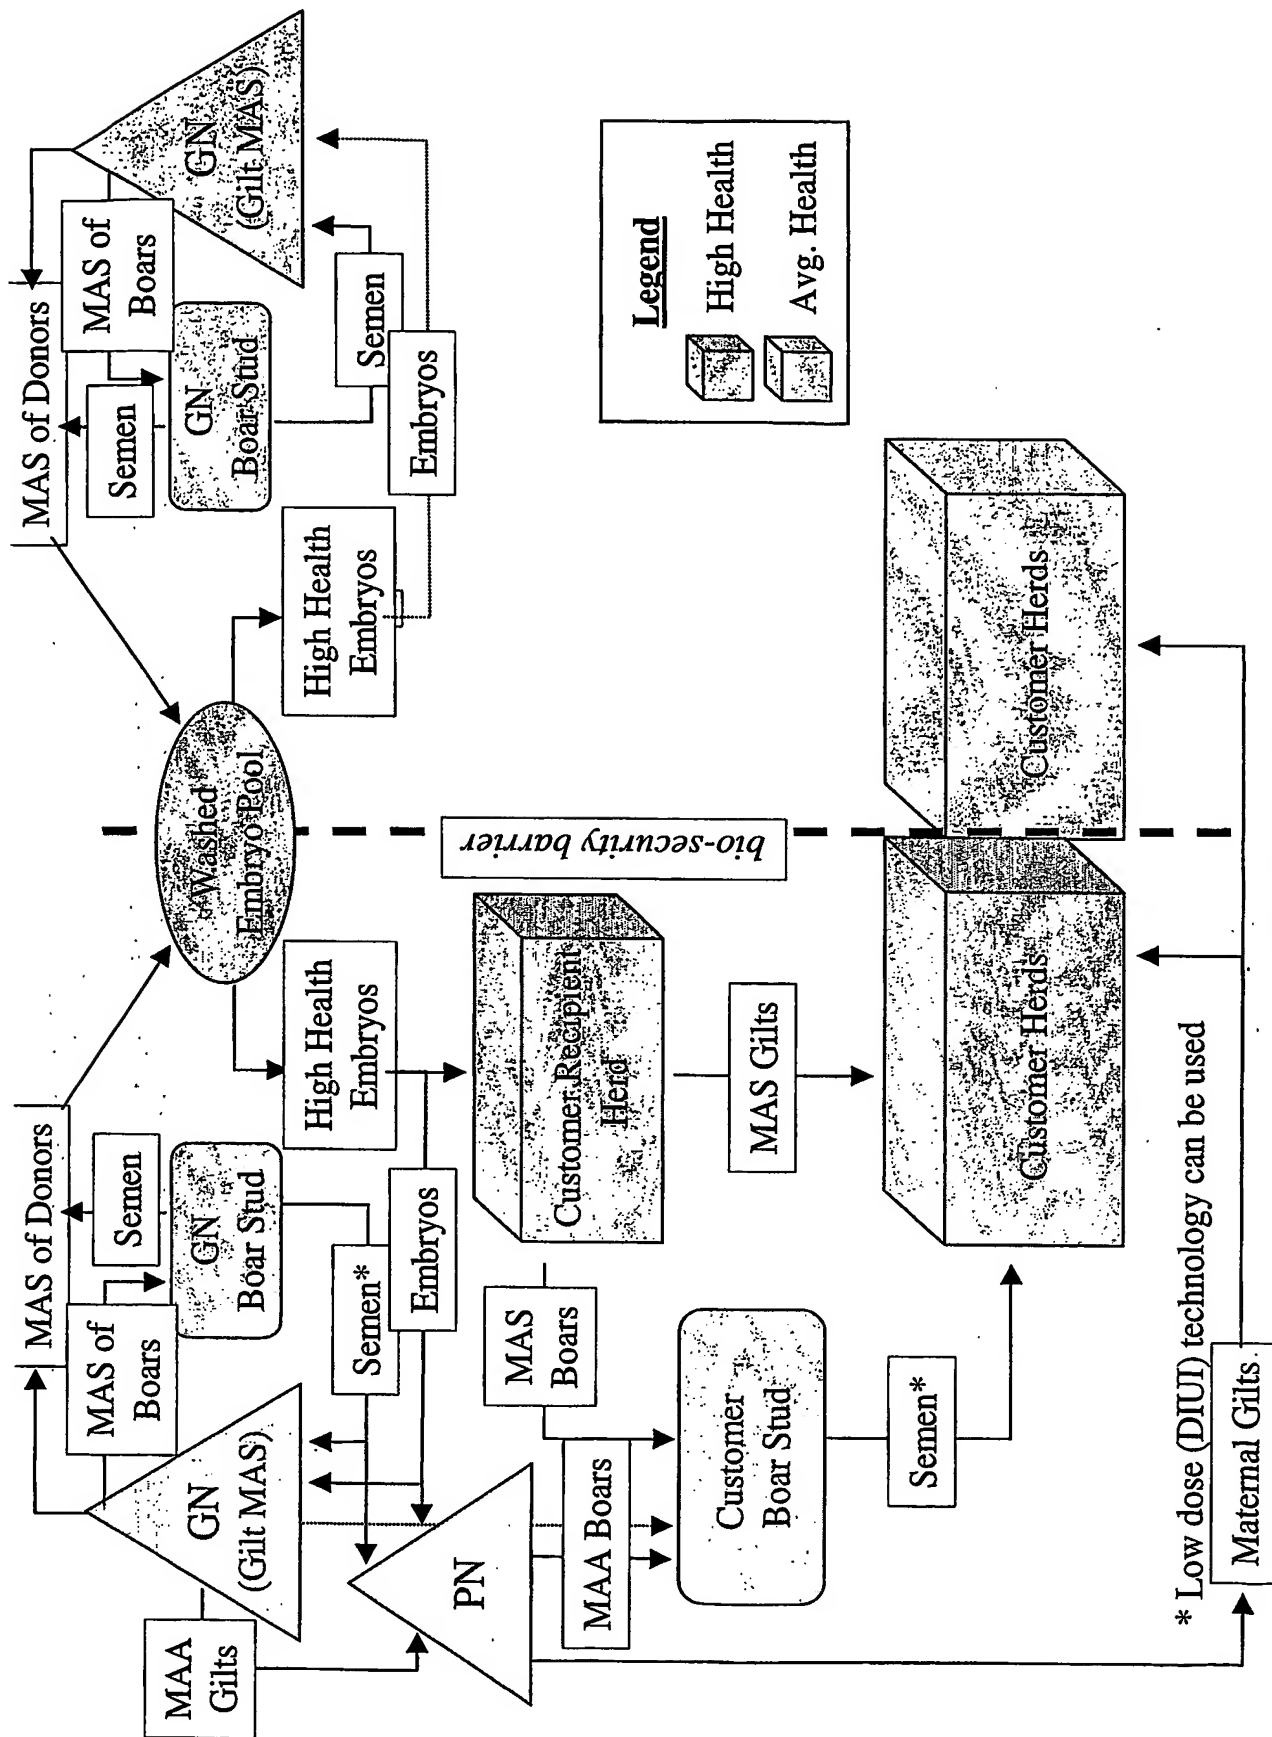


FIGURE 15

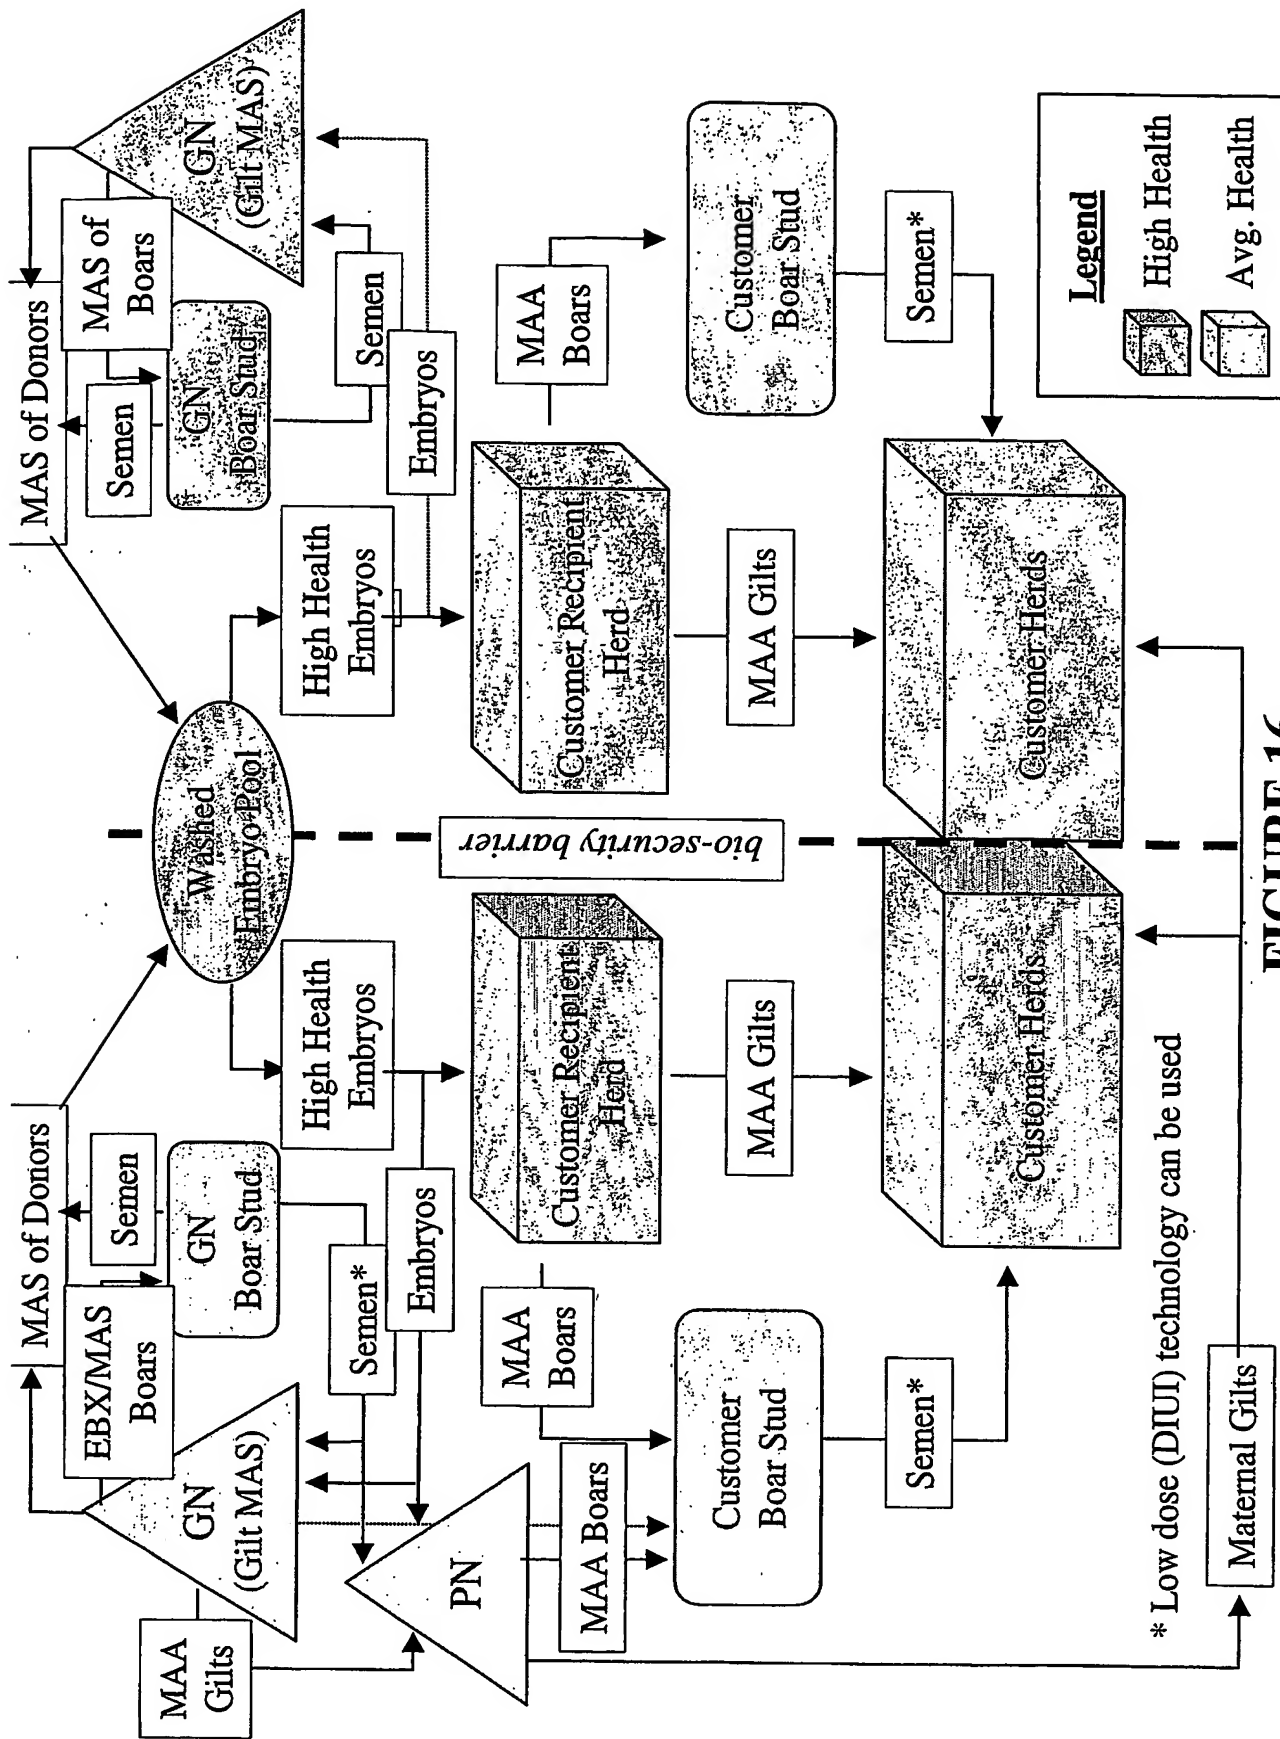


FIGURE 16